

Sample Received: July 16, 2026

COA Issued: July 31, 2026

PRODUCT INFORMATION

Vendor: AubX Sample Name: KLOW 80mg Sample Type: Blue lyophilized powder Lot Number: AX-KL-00001 MW (g/mol): 403.2, 342.4, 1419.5, 4964.2



ANALYTICAL METHODS

Identity: Confirmed via LC-MS/MS
Purity: RP-HPLC (214 nm)
Content: HPLC quantitation

TEST RESULTS

Specification	Result	Method	Status
Identity: KLOW	GHK-Cu, KPV, BPC-157, TB-500	LC-MS/MS	✓ Conforms
Content	51.61, 10.48, 10.67, 10.25 mg	HPLC Quantitation	✓ Conforms
Overall Purity	99.8%	RP-HPLC (214 nm)	✓ Conforms

HPLC Chromatogram (Retention Time: 1.940, 2.319, 9.146, 9.230 min)

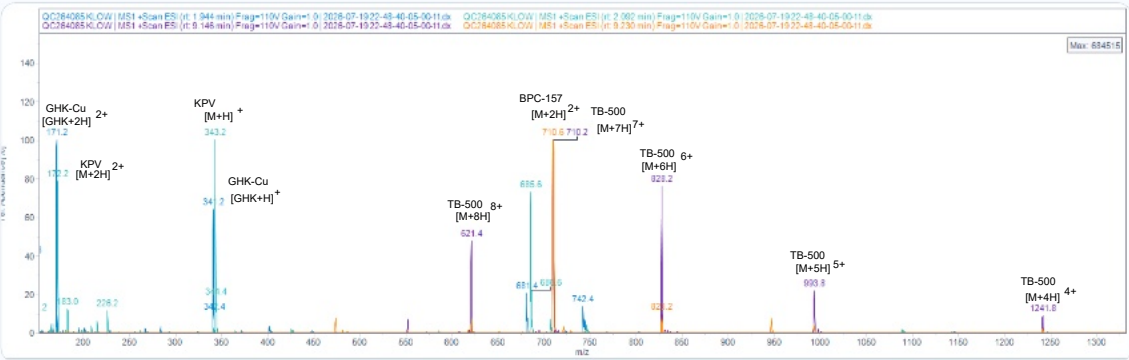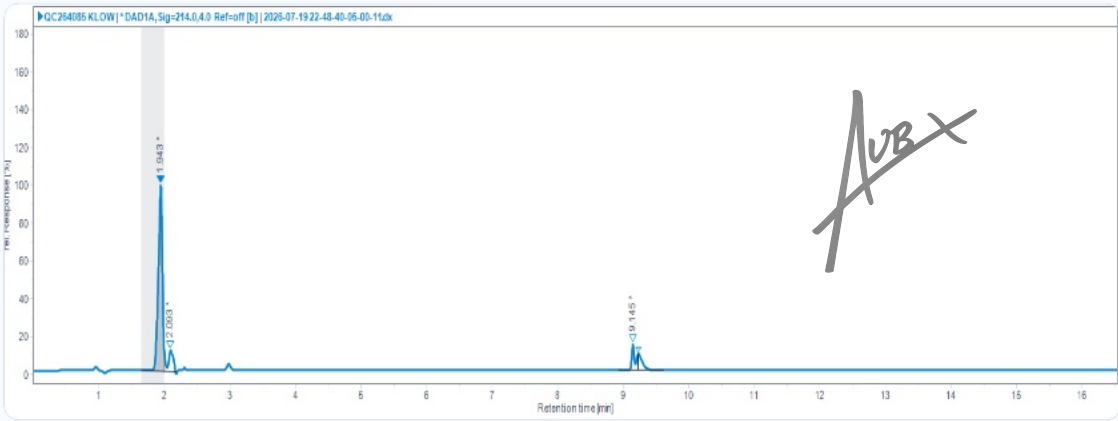

Certification: This COA confirms that the tested material meets or exceeds Bioviridian’s analytical quality specifications for peptide research use.
Visit: <https://bioviridians.com/coa-search.html>



Shane Straight
Shane Straight, M.S.
Principal Chemist, Bioviridian Inc.